

Containers

#	Product Code	Product Description	Liner Bag Type	Solidifying Agent	Flow Stopper	Quantity
①	DKI-FF2861	1 Liter Final Liner Bag without solidifying agent	Thick Plastic Type		○	10 pcs × 5 sets/box
②	DKI-FF861	1 Liter Final Liner Bag with solidifying agent	Thick Plastic Type	○	○	10 pcs × 5 sets/box
③	DKI-RD4862P	2 Liter Pre Liner Bag without solidifying agent	Thick Plastic Type			10 pcs × 5 sets/box
④	DKI-RD862P	2 Liter Pre Liner Bag with solidifying agent	Thick Plastic Type	○		10 pcs × 5 sets/box
⑤	DKI-RD4862F	2 Liter Final Liner Bag without solidifying agent	Thick Plastic Type		○	10 pcs × 5 sets/box
⑥	DKI-RD862F	2 Liter Final Liner Bag with solidifying agent	Thick Plastic Type	○	○	10 pcs × 5 sets/box
⑦	DKI-TF4020P	2 Liter Pre Liner Bag without solidifying agent	Film Type			5 pcs × 10 sets/box
⑧	DKI-TF3020P	2 Liter Pre Liner Bag with solidifying agent	Film Type	○		5 pcs × 10 sets/box
⑨	DKI-TF4020F	2 Liter Final Liner Bag without solidifying agent	Film Type		○	5 pcs × 10 sets/box
⑩	DKI-TF3020F	2 Liter Final Liner Bag with solidifying agent	Film Type	○	○	5 pcs × 10 sets/box
⑪	DKI-TF4035P	3.5 Liter Pre Liner Bag without solidifying agent	Film Type			5 pcs × 10 sets/box
⑫	DKI-TF3035P	3.5 Liter Pre Liner Bag with solidifying agent	Film Type	○		5 pcs × 10 sets/box
⑬	DKI-TF4035F	3.5 Liter Final Liner Bag without solidifying agent	Film Type		○	5 pcs × 10 sets/box
⑭	DKI-TF3035F	3.5 Liter Final Liner Bag with solidifying agent	Film Type	○	○	5 pcs × 10 sets/box

Accessories

#	Product Code	Product Description	Quantity	Product Description
⑮	DKI-FF7301	Canister for 1 Liter	1 pc	Bag Type for 1 Liter
⑯	DKI-RD730P	Canister for 2 Liter Pre	1 pc	Bag Type for 2 Liter Pre
⑰	DKI-RD730F	Canister for 2 Liter Final	1 pc	Bag Type for 2 Liter Final
⑱	DKI-FF7303	Canister for 3.5 Liter Pre/Final	1 pc	Bag Type for 3.5 Liter(Pre・Final)
⑲	DKI-FF707(H)	FF Caster Set for Bag(High)	1 set	Caster(High) + Canister for 2 Liter Pre(3pcs) + Canister for 2 Liter(1pc)
⑳	DKI-FF707(L)	FF Caster Set for Bag(Low)	1 set	Caster(Low) + Canister for 2 Liter Pre(3pcs) + Canister for 2 Liter(1pc)
㉑	DKI-FF708H	FF Caster Set for 3.5 Liter(High)	1 set	Caster(High) + Canister for 3.5 Liter Pre(2pcs)
㉒	DKI-FF704(H)	Caster(High)	1 stand	High for Bag Type
㉓	DKI-FF704(L)	Caster(Low)	1 stand	Low for Bag Type
㉔	DKI-FF704H10	Caster(High) (Disassembled Type)	1 set	10 Disassembled Caster in 1 carton
㉕	DKI-FF765	FF 1 L Wall Hanging Set	1 set	Canister for 1 Litter + Hook for Canister
㉖	DKI-FF767	FF 2 L Wall Hanging Set	1 set	Canister for 2 Litter + Hook for Canister
㉗	DKI-RD792	Wall Hanging Hook for Canister	1 pc	Wall Hanging
㉘	RG-300	FitFix Regulator	1 pc	* RG-300 is not a CE marked product.
㉙	DKI-FF704K	Trestle for Regulator	1 pc	Trestle for Regulator
㉚	DKI-RD886	Three way stopcock	1 pc	Suction way switch valve
㉛	DKI-RD890	Nipple with bowl valve	1 pc	Switch valve
㉜	DKI-RD795	Caster Hook for Canister	1 pc	Caster Hook

Expendables

#	Product Code	Product Description	Quantity	Product Description
③③	DKI-RD920	Solidifying agent bottle	30 bottles	1 bottle: 220g
③④	DKI-RD888	Inlet elbow	120 pcs	White
③⑤	DKI-RD841	Flow stopper	30 pcs	Overflow Protection



*For ICU & NICU

How to set-up &
How to use
video available



https://www.daiken-iki.co.jp/en/pi/seihin_ff.html



Pioneering the future of medical technology

DAIKEN MEDICAL CO., LTD.

International Department: 2-6-2, Ayumino, Izumi-city,
Osaka, 594-1157, Japan

COOPDECH's product information is available at the corporate website.
<http://www.daiken-iki.co.jp/>

[Agency]

2022.1

Contents of this catalog are as of January 2022.



COOPDECH

COOPDECH FitFix™ (Disposable Suction Container System)

- Strong and consistent suction system
- Safe handling of medical waste by using solidifying agent
- Available with or without solidifying agent
- Easy to handle
- Compact footprint
- Variety of configurations



DAIKEN MEDICAL CO., LTD.



Disposable Suction Bag FitFix™



Infection Control with Safety New Standard for Medical Suctioning Device

“FitFix” SUCTION CONTAINER SYSTEM


The safest & the most widely used medical disposable suction system in Japan.

- Daiken Medical offers a complete set of fluid management products to provide everything you need. Our single-use systems deliver exceptional performance and provide hygienic, safe and efficient disposal of liquid waste.
- Completely closed system and the solidifying agent integrated on top of the liner bag, allows healthcare workers to handle the biological liquid waste without exposure.
- A one-way valve and hydrophobic shut-off filter perform the function of overflow valve, by stopping the suction when the maximum level of filling has been reached.
- A graduated scale, printed on the external canister, allow the monitoring of the volume of collected fluid.



Single Wall-mounted Type

Liner Bag 1.0 L Thick Plastic Type

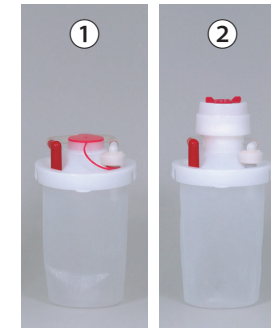


①DKI-FF2861 ②DKI-FF861

Liner Bag 2.0 L Thick Plastic Type




③DKI-RD4862P ④DKI-RD862P

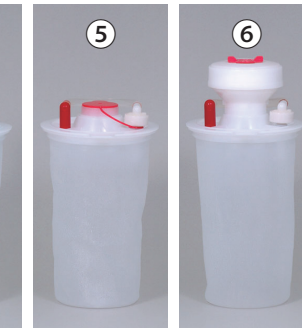

⑤DKI-RD4862F ⑥DKI-RD862F

Liner Bag 2.0 L Film Type

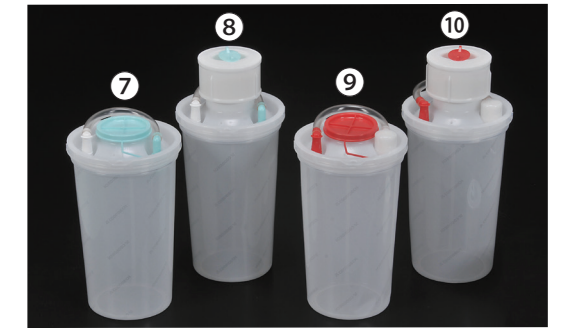


⑦DKI-TF4020P ⑧DKI-TF3020P
⑨DKI-TF4020F ⑩DKI-TF3020F

Liner Bag 3.5 L Film Type




⑪DKI-TF4035P ⑫DKI-TF3035P
⑬DKI-TF4035F ⑭DKI-TF3035F

Canister

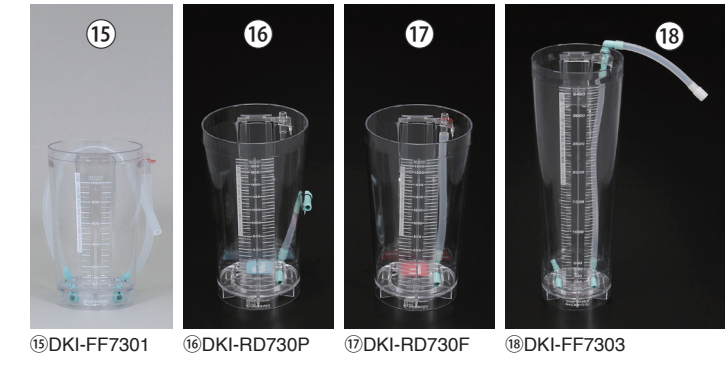


⑮DKI-FF7301 ⑯DKI-RD730P ⑰DKI-RD730F ⑱DKI-FF7303

Caster Set

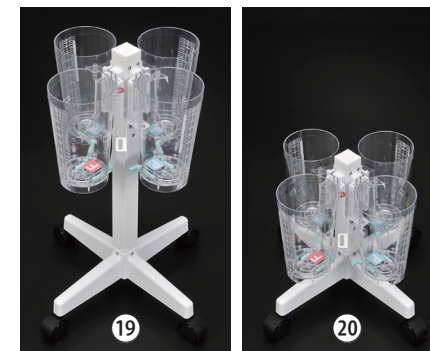

⑲DKI-FF707(H) ⑳DKI-FF707(L) ㉑DKI-FF708H

Caster

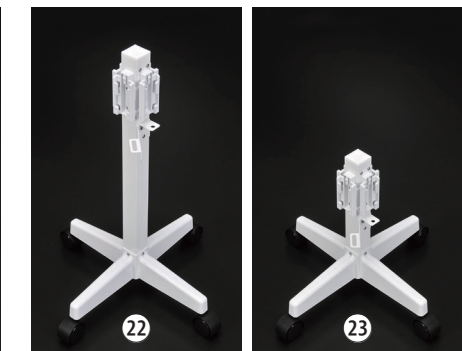

㉒DKI-FF704(H) ㉓DKI-FF704(L)

Disassembled Type




㉔DKI-FF704H10

Wall Hanging Set




㉕DKI-FF765 ㉖DKI-FF767 ㉗DKI-RD792

Others

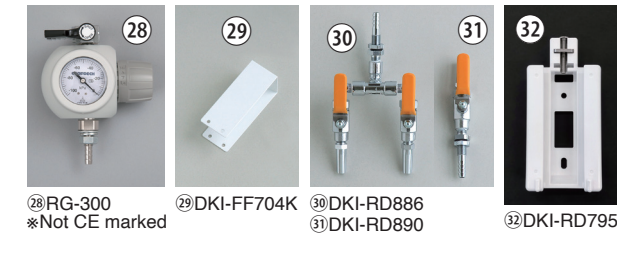

㉘RG-300
*Not CE marked ㉙DKI-FF704K ㉚DKI-RD886
㉛DKI-RD890 ㉜DKI-RD795

Expendables

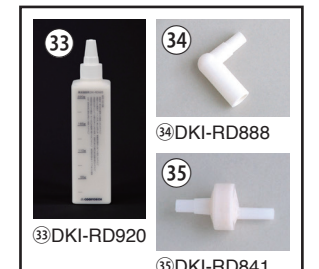

㉝DKI-RD920 ㉞DKI-RD888
㉟DKI-RD841

Procedures:

Setting up the Liner Bag



Pull up the liner bag.



Set each liner bag firmly to the canisters. For the Pre liner bags, connect the vacuum tube set to the patient port seated next to each liner. For Final liner bag, connect the inlet elbow to its connector.



Attach the connecting tube to the patient port on the FitFix Liner pre#1 and start suctioning.

Detaching the Liner Bag



After suctioning, connect the inlet port to its own Inlet and seal it firmly.



Disperse the solidifying agent by rotating the plunger 90 degrees, then push it downwards.



After confirming the suction fluid is solidified, remove the liner bag from the canister.